

## DENTAL SURGICAL INSTRUMENT KIT








# GDT FIXTURE REMOVER KIT

### INSTRUCTIONS FOR USE

#### DESCRIPTION

The device is intended for use in removing failed implanted fixture.

#### CONTENT


Product	Type	H (mm)
	x2 Fixture remover screw Ø 1.6 / 1.8	22.0
	x2 Fixture remover screw Ø 2.0 / 2.5	22.0
	Fixture remover screw Narrow	22.0
	Ratchet extension Ø 6.0	16.0
	Handpiece condenser Ø 6.0	24.0
	Wrench Long	110.0
	Turning Handle	11.0

## HOW TO USE

### Removing Fixture

Drill the Fixture Remover Screw counterclockwise to fix the remover to the implanted fixture and keep drilling counterclockwise to remove the fixture. \* *In case the Fixture Remover Screw cannot be separated from the fixture due to excessive torque, use the forceps or mini vise to turn the screw clockwise.*

- Turning Handle and Wrench-Long are used to turn Fixture Remover Screw manually.
- Ratchet Extension is used to extend the length of Fixture Remover Screw when the surgical site is not accessible.
- Handpiece Condenser is used to connect Fixture Remover Screw to the implant engine.

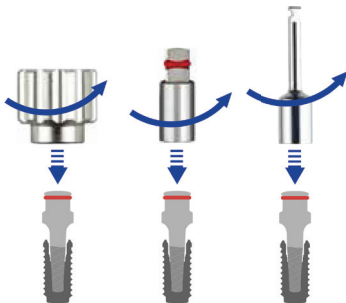

### STORAGE AND TRANSPORTATION CONDITIONS

The device should be kept during storage and transportation at room temperature in dry place. Keep the device out of direct sunlight and avoid heavy materials placing on the device.

### WARNING

- For efficient and safe use of this device, the surgeon should be sufficiently trained and have enough experience in surgical operation technique related to these instruments.
- The surgeon is responsible for making reasonable judgement on deciding which instrument and surgical technique to use for a special purpose considering condition of individual patient.

### CAUTIONS

- The surgeon should be well acquainted with suitable precautions against problems that may occur during an operation.

- Excessive drilling can cause injury during surgical operation.

## **PRECAUTIONS**

- The surgeon should inform the patient of the risks associated with surgery.
- Inspect each device to ensure they are not damaged.
- All instruments must be sterilized prior to use.
- The device should be used by sufficiently trained surgeon.
- The device should not be modified or used against the [Indications for Use] stated in this document.

## **POSSIBLE ADVERSE EFFECTS**

Allergy to metallic material, inflammation and/or infection caused by carelessness.

## **CONTRAINDICATION**

- Do not use for the patients with active or suspected infection, immune deficiency history, steroid treatment, bleeding disorder, endocrine diseases, osteomyelitis or other acute diseases and the patients receiving radiation therapy on the cranium or having gingival diseases or severe oral hygiene problems unless the surgeon make reasonable judgement that the surgery with the device is safe for the patients under appropriate control.
- Do not use for any patient who is not suitable for surgery including the patients with allergy to metallic material.

## **CLEANING & STERILIZATION**

The subject devices, surgical instruments, are reusable after cleaning and sterilizing. They must be cleaned before reuse. Following these recommended instructions for cleaning.

### **1) Cleaning:**

- ① Disassemble the device where possible.
- ② Remove body fluids or blood with flowing water.
- ③ Cleanse the device thoroughly using suitable brushes in flowing water until foreign substances are removed. (do not use metal brushes or steel wool).

- ④ Cleanse the device with surgical instrument cleaner according to the instructions provided by the manufacturer of the cleaner.
- ⑤ Rinse the device in flowing water or distilled water for 20 seconds three times.
- ⑥ Air-dry or wipe the device with clean cloth and alcohol to prevent from water spot.

## 2) Pre-Cleaning:

- ① Follow the same instructions from ④ to ⑥ of Cleaning.

## 3) Sterilization:

Dental Surgical Instruments is supplied NON-STERILE.

They must be sterilized by the end user after and prior to use.

Only legally marketed, FDA-cleared sterilization barriers (e.g. wraps or pouches) should be used.

## MATERIAL

Stainless Steel, Silicone ring.



Global Dental Transfer.  
Yitzhak Ben Zvi 9/64, Beer Sheva,  
Israel.  
Tel: +972.54.77.90.282  
e-mail: info@gdt-Implants.com  
www.gdentalt.com

## PACKAGING

The device is packaged in KIT.

This device is manufactured made for GDT Implants.

## Ref: SD-FR

Consult instructions for use



Manufacturer



Caution



Reference / Article number



Non-sterile product



Batch Code



Temperature limitation



Date of manufacture



Keep away from rain



Symbol for "Use by  
Prescription only"

**Rx Only**

Keep away from sunlight



*The manufacturer is not responsible for any loss of quality caused by the failure to comply with terms of transportation, storage and use established by the manufacturer for this product. Responsibility for the use of the material for purposes other than those specified by the manufacturer falls on the user.*